

Proper Fit **Every Time**

To ensure a proper fit, it is crucial to measure the stoma length using the AMT Balloon Stoma Measuring Device.

BALLOON STOMA MEASURING DEVICE	ORDER #	QTY/BOX
GUIDEWIRE COMPATIBLE	1804	10
NON-GUIDEWIRE COMPATIBLE	1704	10

MiniONE® Button

Low Profile Balloon Gastrostomy Tube

MiniONE® Balloon Button

AMT®	12 F		14 F		16 F		18 F		20 F		24 F	
LENGTH cm	ORDER NUMBERS											
	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®
0.8	M1-5-1208	M1-5-1208-I	M1-5-1408	M1-5-1408-I								
1.0	M1-5-1210	M1-5-1210-I	M1-5-1410	M1-5-1410-I	M1-5-1610	M1-5-1610-I	M1-5-1810	M1-5-1810-I	M1-5-2010	M1-5-2010-I		
1.2	M1-5-1212	M1-5-1212-I	M1-5-1412	M1-5-1412-I	M1-5-1612	M1-5-1612-I	M1-5-1812	M1-5-1812-I	M1-5-2012	M1-5-2012-I		
1.5	M1-5-1215	M1-5-1215-I	M1-5-1415	M1-5-1415-I	M1-5-1615	M1-5-1615-I	M1-5-1815	M1-5-1815-I	M1-5-2015	M1-5-2015-I	M1-5-2415	M1-5-2415-I
1.7	M1-5-1217	M1-5-1217-I	M1-5-1417	M1-5-1417-I	M1-5-1617	M1-5-1617-I	M1-5-1817	M1-5-1817-I	M1-5-2017	M1-5-2017-I	M1-5-2417	M1-5-2417-I
2.0	M1-5-1220	M1-5-1220-I	M1-5-1420	M1-5-1420-I	M1-5-1620	M1-5-1620-I	M1-5-1820	M1-5-1820-I	M1-5-2020	M1-5-2020-I	M1-5-2420	M1-5-2420-I
2.3	M1-5-1223	M1-5-1223-I	M1-5-1423	M1-5-1423-I	M1-5-1623	M1-5-1623-I	M1-5-1823	M1-5-1823-I	M1-5-2023	M1-5-2023-I	M1-5-2423	M1-5-2423-I
2.5	M1-5-1225	M1-5-1225-I	M1-5-1425	M1-5-1425-I	M1-5-1625	M1-5-1625-I	M1-5-1825	M1-5-1825-I	M1-5-2025	M1-5-2025-I	M1-5-2425	M1-5-2425-I
2.7	M1-5-1227	M1-5-1227-I	M1-5-1427	M1-5-1427-I	M1-5-1627	M1-5-1627-I	M1-5-1827	M1-5-1827-I	M1-5-2027	M1-5-2027-I	M1-5-2427	M1-5-2427-I
3.0	M1-5-1230	M1-5-1230-I	M1-5-1430	M1-5-1430-I	M1-5-1630	M1-5-1630-I	M1-5-1830	M1-5-1830-I	M1-5-2030	M1-5-2030-I	M1-5-2430	M1-5-2430-I
3.5	M1-5-1235	M1-5-1235-I	M1-5-1435	M1-5-1435-I	M1-5-1635	M1-5-1635-I	M1-5-1835	M1-5-1835-I	M1-5-2035	M1-5-2035-I	M1-5-2435	M1-5-2435-I
4.0	M1-5-1240	M1-5-1240-I	M1-5-1440	M1-5-1440-I	M1-5-1640	M1-5-1640-I	M1-5-1840	M1-5-1840-I	M1-5-2040	M1-5-2040-I	M1-5-2440	M1-5-2440-I
4.4			M1-5-1444	M1-5-1444-I	M1-5-1644	M1-5-1644-I	M1-5-1844	M1-5-1844-I	M1-5-2044	M1-5-2044-I	M1-5-2444	M1-5-2444-I
5.0			M1-5-1450	M1-5-1450-I	M1-5-1650	M1-5-1650-I	M1-5-1850	M1-5-1850-I	M1-5-2050	M1-5-2050-I	M1-5-2450	M1-5-2450-I
5.5			M1-5-1455	M1-5-1455-I	M1-5-1655	M1-5-1655-I	M1-5-1855	M1-5-1855-I	M1-5-2055	M1-5-2055-I	M1-5-2455	M1-5-2455-I
6.0			M1-5-1460	M1-5-1460-I	M1-5-1660	M1-5-1660-I	M1-5-1860	M1-5-1860-I	M1-5-2060	M1-5-2060-I	M1-5-2460	M1-5-2460-I
6.5			M1-5-1465	M1-5-1465-I								
7.0			M1-5-1470	M1-5-1470-I								
8.0			M1-5-1480	M1-5-1480-I								
9.0			M1-5-1490	M1-5-1490-I								
10.0			M1-5-14100	M1-5-14100-I								

*The MiniONE® Balloon Button comes packaged as 1/box.

Feed Sets Included in Kit



Complete Portfolio | Extension Sets


ADAPTER OPTIONS	RIGHT ANGLE CONNECTOR OPTIONS			STRAIGHT CONNECTOR OPTIONS		
	2"	12"	24"	2"	12"	24"
Purple Bolus		8-1221	8-2421	8-0211	8-1211	8-2411
Clear Y-Port XL	8-0222	8-1222	8-2422	8-0212	8-1212	
Purple Y-Port		8-1257G† 8-1255	8-2455			
Single ENFit®		8-1221-ISOSAF 8-1223-ISOSAF 8-1226-ISOSAF	8-2421-ISOSAF 8-2423-ISOSAF	8-0211-ISOSAF	8-1211-ISOSAF	8-2411-ISOSAF
Dual ENFit®	8-0222-ISOSAF	8-1222-ISOSAF 8-1255-ISOSAF	8-2422-ISOSAF 8-2455-ISOSAF	8-0212-ISOSAF	8-1212-ISOSAF	

†Y-Port with enhanced med port plug. Feed sets come packaged as 10/box. Not Made with PVC: 8-1255-ISOSAF-NP, 8-2455-ISOSAF-NP and 8-1211-ISOSAF-NP. To ensure optimal performance and reliability, AMT recommends the exclusive use of AMT extension sets with AMT devices. Although other brands may appear compatible, AMT cannot guarantee their safety, performance, or durability when used in place of AMT extension sets.

Balloon Fill Volumes

FRENCH SIZE	MIN	REC.	MAX
12F	2 ml	2.5 ml	3 ml
14F	3 ml	4 ml	5 ml
16F	4 ml	6 ml	8 ml
18F	6 ml	8 ml	10 ml
20F	7 ml	10 ml	15 ml
24F	7 ml	10 ml	15 ml

Recommended water fill volume is clearly printed on each MiniONE® Balloon Button fill valve. Consult your healthcare provider before adjusting fill volumes.

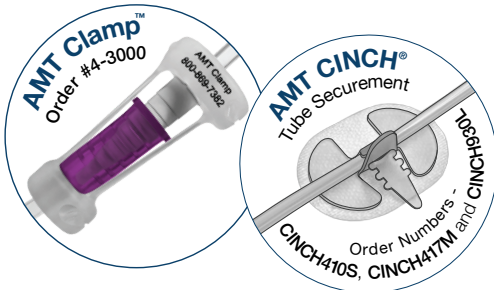

Reduce Leaks

Improve Comfort

Soft + Flexible

Glow Green™ Technology

For a complete list of products, visit us at www.AppliedMedical.net
800 869 7382 | CS@AppliedMedical.net | ICS@AppliedMedical.net



Applied Medical Technology, Inc.
8006 Katherine Boulevard
Brecksville, OH 44141
www.AppliedMedical.net
An ISO 13485 Registered Company
Cleared For Initial Placement
MR Conditional
Made In USA



Innovating. Educating. Changing Lives.™

© 2025 Applied Medical Technology, Inc. C-3922-P
Patents: <http://www.AppliedMedical.net/Patents/> | Trademarks: <http://www.AppliedMedical.net/Trademarks/>
ENFit® is a registered trademark of GEDSA. | 1.Claims based on internal testing of 14F devices.


AMT MiniONE® Balloon Button



Exclusive AMT Balloon
Superior Gastric Seal



Soft + Flexible
Optimized for Comfort

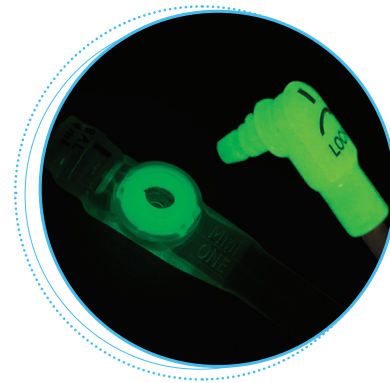

Glow Green™
Easier Nighttime Feeds

An Advantage in Enteral Nutrition

Reduce Leaks

The MiniONE® Balloon Button was designed to reduce gastric leakage that can cause nutrient loss, skin damage, and granulation tissue

- **Exclusive AMT Balloon**
apple-shaped, expands horizontally
>50% more internal stoma coverage¹
- **Tapered Transition**
from bolster to tube, for a more secure fit
- **Anti-Reflux Valve**
prevents backflow
- **Adjustable Balloon Volume**
ensures proper fit


Soft + Flexible

- **Flexible External Bolster**
easy to clean around the stoma site
- **Balloon Fill Port**
angled away from the body to reduce skin irritation at the stoma site
- **Gentle to the Skin**
designed to reduce granulation tissue

Improve Comfort

AMT understands that comfort is key when it comes to patient, caregiver and clinician satisfaction

- **37% Lower External Profile¹**
MiniONE® lays discreetly below clothing
- **30% Lower Balloon Profile¹**
occupies less space within the stomach

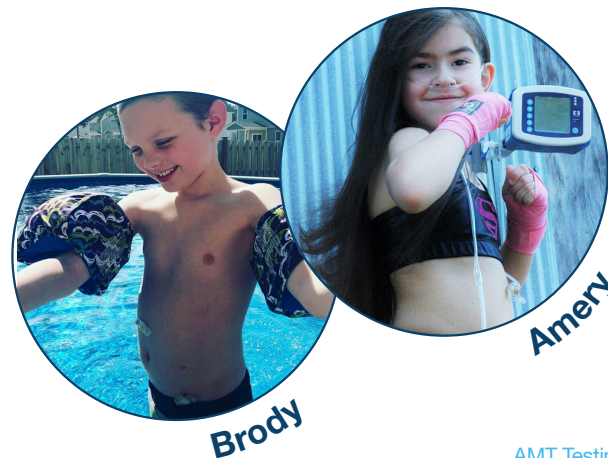


Brody

Amery

AMT Testimonials
[AppliedMedical.net/Stories](https://www.appliedmedical.net/stories)

Your **ONE** Source for Enteral Nutrition Devices. Accessories. Resources. Support.

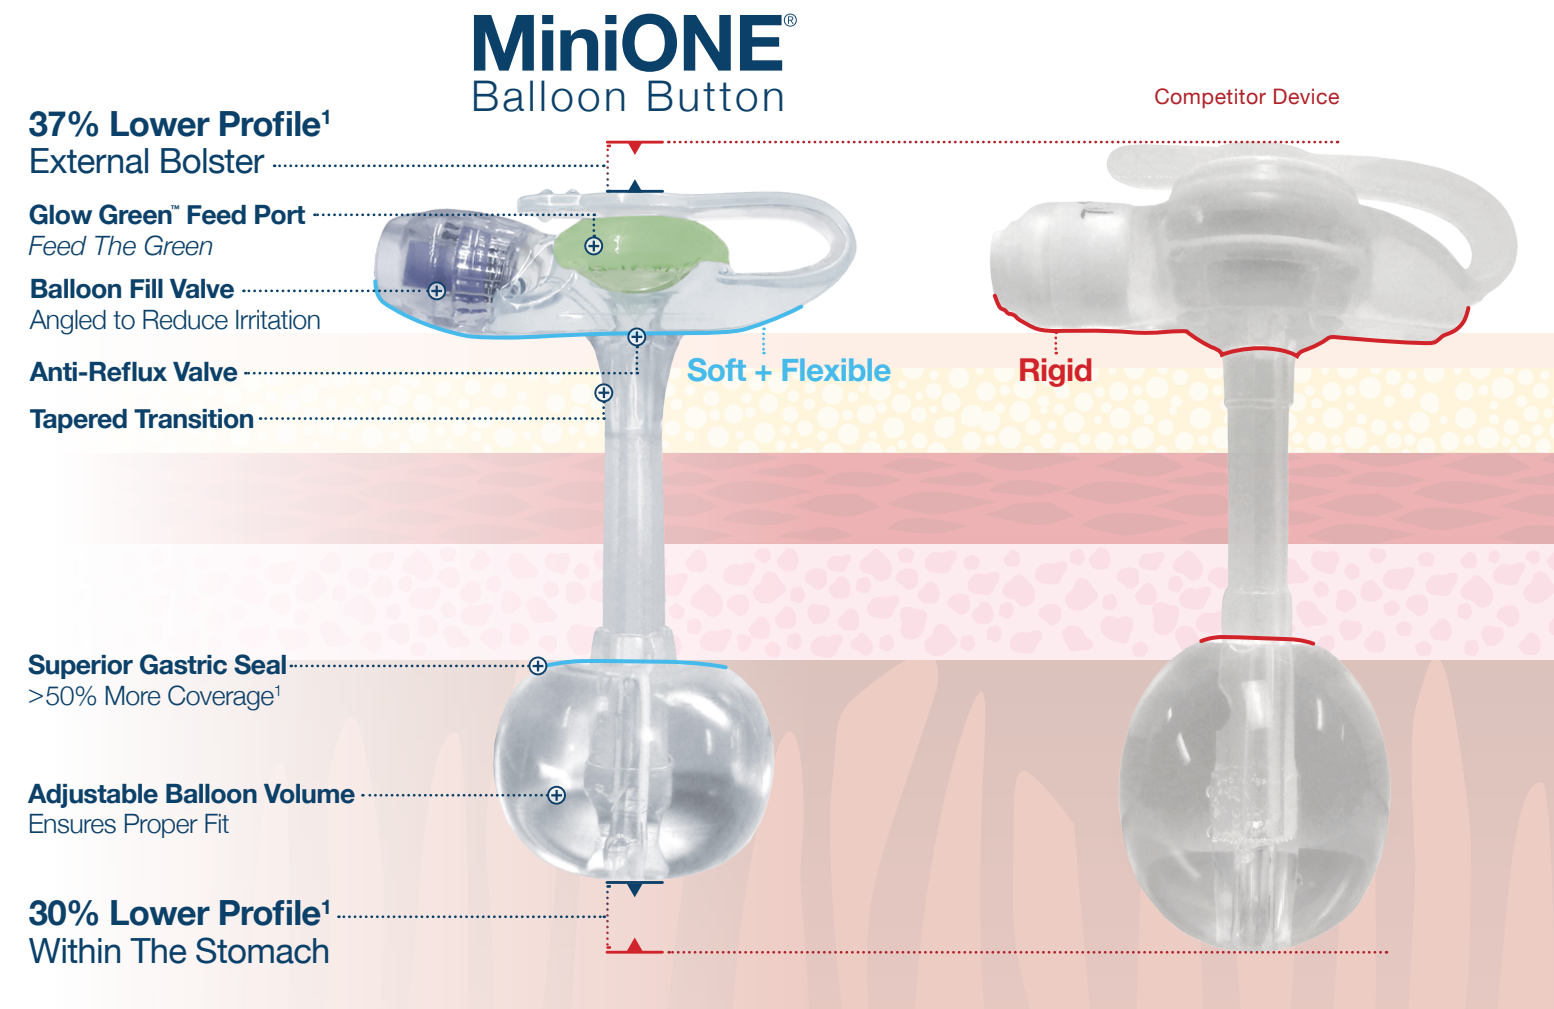

Safe + Secure Feed Set Attachment

To attach a feed set to a MiniONE® Balloon Button, follow these easy steps:

