



CINCH[®]

Tube Securement Device


Small CINCH[®]
4F to 10F

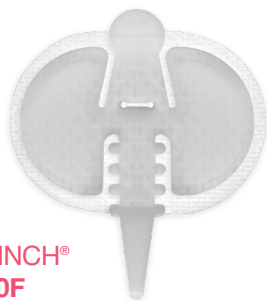

Medium CINCH[®]
4F to 17F

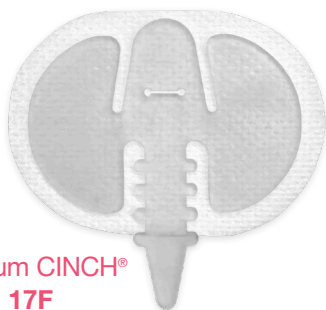

Large CINCH[®]
9F to 30F

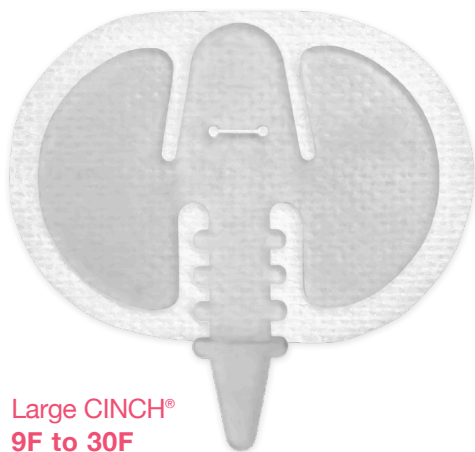

Patient Comfort First

The low profile and flexible design allows for comfort and mobility.

Safe + Secure

Anchors medical tubes while relieving stress and strain at insertion points.

Hypoallergenic Adhesive

Provides gentle yet secure attachment.

Easy to Use

Simply clean the skin, apply the CINCH[®], and secure the tube!

NEW! The CINCH[®] Family Now Includes Three Sizes!



Innovating. Educating. Changing Lives.™

800 869 7382 | CS@AppliedMedical.net | ICS@AppliedMedical.net

CINCH®

From 4F to 30F, the CINCH® Has You Covered!

Versatile

Small CINCH® secures tubes 4F to 10F,
Medium CINCH® secures tubes 4F to 17F,
Large CINCH® secures tubes 9F to 30F.

Comfortable

Soft, low-profile, flexible.

Breathable Backing


In three convenient sizes:
Small (1 cm x 1.5 cm),
Medium (3 cm x 4 cm),
Large (4 cm x 6 cm).

Hypoallergenic

Gentle adhesive for sensitive skin.



Reusable

Elastomer strap can be repeatedly opened and closed.

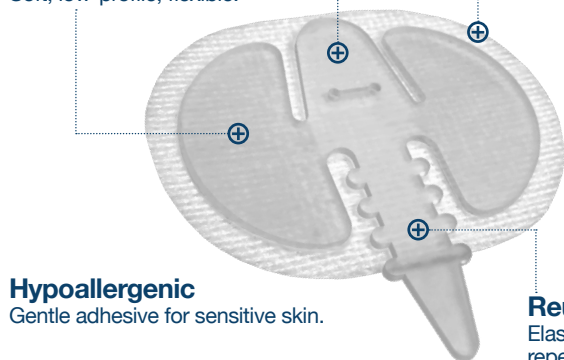

Front


Back



The CINCH® comes fully assembled with an easy-peel split backing.

Small CINCH®

4F




10F



Medium CINCH®

4F




17F




Large CINCH®

9F

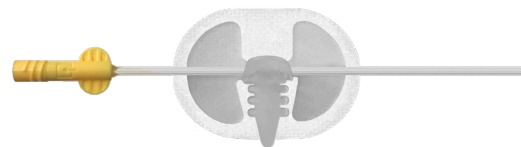

30F

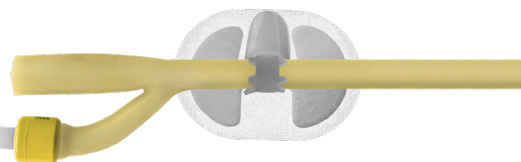

CINCH® | Order Information

Description	Tube Securement Range	Qty/Box	Order Number
Small CINCH®	4F to 10F	10	CINCH410S-10
		50	CINCH410S-50
Medium CINCH®	4F to 17F	10	CINCH417M-10
		50	CINCH417M-50
Large CINCH®	9F to 30F	10	CINCH930L-10
		50	CINCH930L-50

For a complete list of products, visit us at www.AppliedMedical.net
800 869 7382 | CS@AppliedMedical.net | ICS@AppliedMedical.net



CINCH® Tube Securement Device



Applied Medical Technology, Inc.
8006 Katherine Boulevard
Brecksville, OH 44141
www.AppliedMedical.net
An ISO 13485 Registered Company
Made In USA



© 2026 Applied Medical Technology, Inc. C-4733-C

Patents: <http://www.AppliedMedical.net/Patents/> | Trademarks: <http://www.AppliedMedical.net/Trademarks/>

CAUTION: If redness or irritation occurs, stop use and consult a healthcare professional. Do not over tighten.

This document is not a substitute for the DFU (Directions for Use).