

Proper Fit **Every Time**
To ensure a proper fit, it is crucial to measure the stoma length using the AMT Balloon Stoma Measuring Device.

Balloon Stoma Measuring Device	Order #	Qty/Box
Guidewire Compatible	1804	10
Non-Guidewire Compatible	1704	10

G-JET® Button

Low Profile Gastric-Jejunal Enteral Feeding Tube

G-JET® Button

G	J	14 F	16 F	18 F
LENGTH		LEGACY ORDER NUMBERS*		
1.0 cm	15 cm	GJ-1410-15	GJ-1610-15	
	22 cm	GJ-1410-22	GJ-1610-22	
1.2 cm	15 cm	GJ-1412-15	GJ-1612-15	
	22 cm	GJ-1412-22	GJ-1612-22	GJ-1812-22
	30 cm	GJ-1412-30	GJ-1612-30	GJ-1812-30
1.5 cm	15 cm	GJ-1415-15	GJ-1615-15	
	22 cm	GJ-1415-22	GJ-1615-22	GJ-1815-22
	30 cm	GJ-1415-30	GJ-1615-30	GJ-1815-30
	45 cm	GJ-1415-45	GJ-1615-45	GJ-1815-45
1.7 cm	15 cm	GJ-1417-15	GJ-1617-15	
	22 cm	GJ-1417-22	GJ-1617-22	GJ-1817-22
	30 cm	GJ-1417-30	GJ-1617-30	GJ-1817-30
	45 cm	GJ-1417-45	GJ-1617-45	GJ-1817-45
2.0 cm	22 cm	GJ-1420-22	GJ-1620-22	GJ-1820-22
	30 cm	GJ-1420-30	GJ-1620-30	GJ-1820-30
	45 cm	GJ-1420-45	GJ-1620-45	GJ-1820-45
2.3 cm	22 cm	GJ-1423-22		
	30 cm	GJ-1423-30	GJ-1623-30	GJ-1823-30
	45 cm	GJ-1423-45	GJ-1623-45	GJ-1823-45
2.5 cm	22 cm	GJ-1425-22		
	30 cm	GJ-1425-30	GJ-1625-30	GJ-1825-30
	45 cm	GJ-1425-45	GJ-1625-45	GJ-1825-45
2.7 cm	30 cm	GJ-1427-30	GJ-1627-30	GJ-1827-30
	45 cm	GJ-1427-45	GJ-1627-45	GJ-1827-45
3.0 cm	45 cm	GJ-1430-45	GJ-1630-45	GJ-1830-45
3.5 cm	45 cm	GJ-1435-45	GJ-1635-45	GJ-1835-45
4.0 cm	45 cm	GJ-1440-45	GJ-1640-45	GJ-1840-45
4.4 cm	45 cm	GJ-1444-45	GJ-1644-45	GJ-1844-45
5.0 cm	45 cm	GJ-1450-45	GJ-1650-45	GJ-1850-45
5.5 cm	45 cm	GJ-1455-45	GJ-1655-45	GJ-1855-45
6.0 cm	45 cm	GJ-1460-45	GJ-1660-45	GJ-1860-45
6.5 cm	45 cm	GJ-1465-45	GJ-1665-45	GJ-1865-45
7.0 cm	45 cm	GJ-1470-45	GJ-1670-45	GJ-1870-45

The G-JET® Button is sold Qty/Box 1 (sterile).
NOTE: G-JET® devices should never be cut to custom lengths.
Guidewire available (180 cm): Order Number 4-GW-5
*Add "-I" for ENFit® G-JET® Button kits.


Balloon Fill Volumes

The recommended water volume is clearly printed on the fill valve of each G-JET® Button. Consult your healthcare provider before adjusting the fill volume.

FRENCH SIZE	MIN	REC.	MAX
14F	3 ml	4 ml	5 ml
16F	3 ml	4 ml	5 ml
18F	7 ml	8 ml	9 ml




Extension + Feed Sets Included in Kit

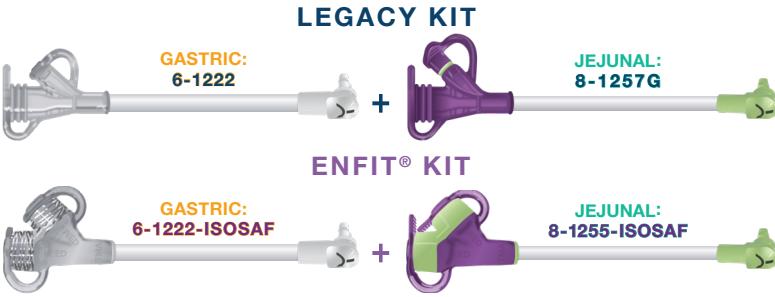

ADAPTERS	RIGHT ANGLE CONNECTORS			STRAIGHT CONNECTORS		
	2"	12"	24"	2"	12"	24"
COMPATIBLE GASTRIC EXTENSION SETS						
Bolus		6-1221	6-2421	6-0211	6-1211	6-2411
Clear Y-Port		6-1222	6-2422	6-0212	6-1212	
ENFit® Y-Port		6-1222-ISOSAF				
COMPATIBLE JEJUNAL FEED SETS						
Purple Y-Port		8-1257G	8-2455			
ENFit® Y-Port	8-0222-ISOSAF	8-1255-ISOSAF	8-2455-ISOSAF	8-0212-ISOSAF		
Bolus		8-1221	8-2421	8-0211	8-1211	8-2411
ENFit® Single Port		8-1221-ISOSAF	8-2421-ISOSAF	8-0211-ISOSAF	8-1211-ISOSAF	8-2411-ISOSAF
Clear Y-Port XL	8-0222	8-1222	8-2422	8-0212	8-1212	

Legacy Included ENFit® Included Extension + Feed sets come packaged as Qty/Box 10.

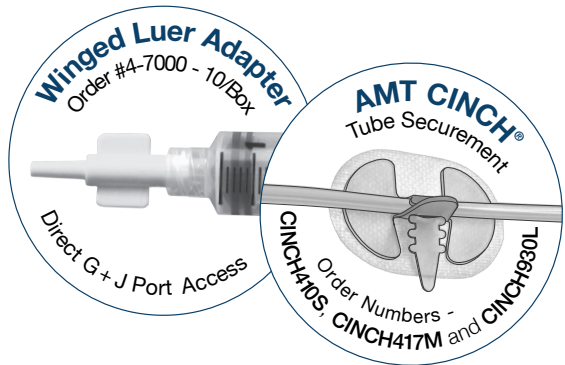

Reduce Clogging
Anti-Kink Technology
AMT Exclusive Balloon
Improve Comfort



Applied Medical Technology, Inc.
8006 Katherine Boulevard
Brecksville, OH 44141
www.AppliedMedical.net
An ISO 13485 Registered Company
Cleared For Initial Placement
Made In USA

© 2026 Applied Medical Technology, Inc. C-4497-P
Patents: <http://www.AppliedMedical.net/Patents/> | Trademarks: <http://www.AppliedMedical.net/Trademarks/>
*The Anti-Reflux Valve is opened when the feed/extension set is locked into place. | ENFit® is a registered trademark of GEDSA.
1.Claim based on internal testing of 14F-22F devices. | 2.Claim based on internal testing of 16F devices.

AMT
Innovating. Educating. Changing Lives.™